

REVIEW

Open Access



# Clinical performance of additively manufactured subperiosteal implants: a systematic review

Eduardo Anitua<sup>1,4\*</sup> , Asier Eguia<sup>2†</sup>, Christoph Staudigl<sup>3</sup> and Mohammad Hamdan Alkhraisat<sup>1,4</sup>

## Abstract

**Purpose** The aim of this study was to assess implant survival and complications rate of modern subperiosteal implants (CAD designed and additively manufactured).

**Methods** A systematic review was conducted using three electronic databases; Medline (Pubmed), Cochrane library, and SCOPUS, following the PRISMA statement recommendations to answer the PICO question: "In patients with bone atrophy (P), do additively manufactured subperiosteal implants (I), compared to subperiosteal implants manufactured following traditional approaches (C), present satisfactory implant survival and complication rates (O)? The study was pre-registered in PROSPERO (CRD42023424211). Included articles quality was assessed using the "NIH quality assessment tools".

**Results** Thirteen articles were finally selected (5 cohort studies and 8 case series), including 227 patients (121 female / 106 male; weighted mean age 62.4 years) and 227 implants. After a weighted mean follow-up time of 21.4 months, 97.8% of implants were in function (5 failures reported), 58 implants (25.6%) presented partial exposure, 12 patients (5.3%) suffered soft tissue or persistent infection. Fracture of the interim prosthesis was reported in 8 of the 155 patients (5.2%) in which the use of a provisional prosthesis was reported. A great heterogeneity was found in terms of study design and methodological aspects. For this reason, a quantitative analysis followed by meta-analysis was not possible.

**Conclusions** Within the limitations of this study, modern additively manufactured subperiosteal implants presented a good survival in the short-time, but a noticeable number of soft-tissue related complications were reported. Further studies are needed to assess the clinical behavior in the medium- and long-term.

**Keywords** Subperiosteal implants, Custom-made implants, Maxillary atrophy, Implant survival

<sup>†</sup>Eduardo Anitua and Asier Eguia contributed equally to the realization of this work.


\*Correspondence:

Eduardo Anitua

[eduardo@fundacioneduardoanitua.org](mailto:eduardo@fundacioneduardoanitua.org)

Full list of author information is available at the end of the article

## Graphical Abstract

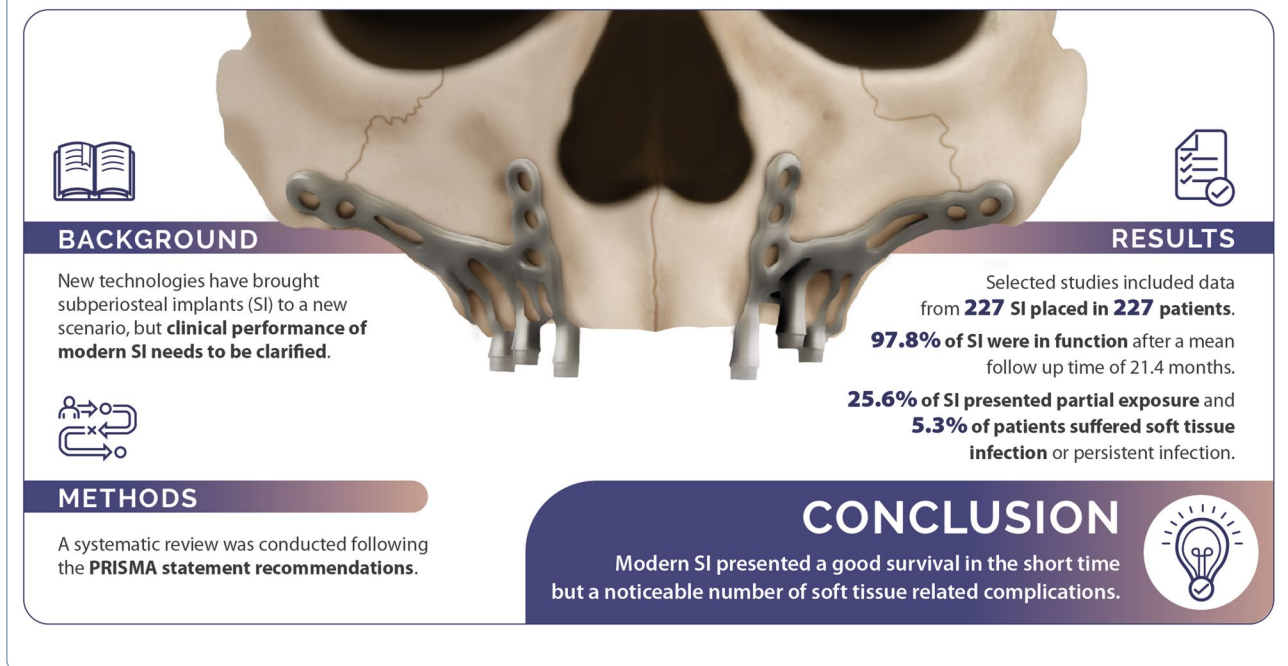

## Introduction

The use of subperiosteal implants (SI) was originally described by Dahl [1] in 1943, but gained relevance after the publication of Goldberg & Gerskoff [2] at the end of the 1940s. In the 1960s the basis of the so-called osseointegration was partially enlightened [3]. This scientific breakthrough, allowed implant dentistry to evolve from an experimental treatment to the current highly predictable option to replace missing teeth [3]. During this step-by-step transformation, SI have evolved like root-shape implants have drastically made. First SI were manufactured in Vitallium [4], (60% cobalt, 20% chromium, 5% molybdenum, and traces of other substances) [5] and were designed to support complete dentures (mostly removable). New SI designs were described and clinically assessed between the 1970s and the late 1990s. [6] At that time, acceptable 5-year results were documented (95% [7, 8] to 100% [9]) but long-term results regarding survival were less favorable (79% at 10 years [7], 76% at 10 years [8], 75% at 6 years [9], 67% at 10 years [10]). A less convenient for the patient two-time surgical approach was also required then. At the first surgery, a wide flap was raised to allow direct analogical bone surface impressions. During the second one, a casted Cr–Co alloy (or others) framework was adapted and placed beneath the mucoperiosteum without anchoring elements (such as osteosynthesis screws) in most of the cases. Lack of

fitting and/or stability, unfavorable biomechanical design, and the use of unsuitable materials to achieve osseointegration, increased the risk of infection, implant exposition, and failure [4, 11]. In case of implant exposition, former SI designs impaired partial or full removal [12]. Probably, this further jeopardized both implant function and esthetics.

SI lost popularity among dental practitioners for a long period, but recent advances in computer-aided design (CAD), computer-aided manufacturing (CAM), the development of new materials (new Ti alloys or Polyether-ether-ketone or PEEK), improvements in surface treatments and a deeper understanding of bone biomechanical principles, have brought SI to a new scenario [13–18]. Thus, modern CAD designed and additively manufactured SI could provide advantages over former SI such as enabling one-time surgery and immediate loading, better fitting or surgical time reduction [14–16].

Frequently, clinicians must face the challenge of treating cases of severe bone atrophy or bone resection. Advances in root-shape implants design and size (short, extra-short and narrow implants) have provided new solutions or have enhanced older ones, for the treatment of different types of bone atrophy [19–21]. Different accessory surgical techniques for recovering the lost bone volume were also developed and improved to treat those patients where root-shape implants could

not be placed directly [22–26]. Among them, guided bone regeneration (GBR), maxillary sinus and nasal floor augmentation, inlay or onlay bone grafting, distraction osteogenesis, nerve lateralization or others have been routinely employed with a varying degree of clinical success [22–26]. The use of zygomatic implants could be also a reliable option for the treatment of those patients with severe posterior maxillary atrophy [27]. The success rate and the incidence and severity of postoperative complications using this type of implants is dependent of clinician expertise [28].

Modern SI have been claimed to present some advantages to treat certain patients with bone atrophy over the above-mentioned techniques. The elimination of bone donor area morbidity (in the case of autologous bone grafting need), the possibility of ambulatory realization and reduction of surgical time, are among the reported benefits for patients [14]. Modern SI also provide an option of treatment for patients with extreme bone defects due to oncologic disease treatment or trauma [29, 30]. On the other hand, the digital resources (devices and software) required to design and manufacture SI are not accessible to all professionals, and the clinical performance of SI is still not well evidenced. This systematic review attempts to assess the clinical performance of modern additively manufactured SI by analyzing their survival and complications rate data available in the literature.

## Materials and methods

A systematic review was carried out following the Preferred Reporting Items for Systematic Reviews and Meta-Analyses (PRISMA) statement recommendations [31] to answer the following the PICO questions: “In patients with bone atrophy (P), do additively manufactured subperiosteal implants (I), compared to subperiosteal implants manufactured following traditional approaches (c), present satisfactory implant survival and complication rates(O)?”. The aim of this review was to answer with the best available evidence, this question to help clinicians when planning the treatment of patients with maxillary or mandibular bone atrophy.

## Protocol and registration

A register in the International Prospective Register of Systematic Reviews (PROSPERO) of the National Institute for Health Research (NIHR) was obtained before starting (CRD42023424211). The PRISMA guidelines for systematic reviews were used to conduct the review process [31].

## Eligibility criteria, information sources and search

Three electronic databases including Medline, Cochrane library, and Scopus were searched. To build the search strategy (PICO), the following considerations were applied:

- *Patient* Patients presenting maxillary or mandibular bone atrophy in the need for oral rehabilitation.
- *Intervention* CAD designed and additively manufactured subperiosteal implant placement (1-time surgical approach).
- *Comparison* Traditional custom-made subperiosteal implants (manufacture of the framework by casting methods; direct impression of bone surface; 2-time surgical approach).
- *Outcomes* Implant survival. Complications rate.

The main question built was then as follows: “In patients with bone atrophy, do additively manufactured subperiosteal implants, compared to subperiosteal implants manufactured following traditional approaches, present satisfactory implant survival and complication rates?”. In the search strategy (Table 1), following terms were employed: “dental implantation, subperiosteal” (MeSH Term) “subperiosteal implant(s)” (free term) and “juxta-osseous implants” (free term). The search query was generated as follows: “dental implantation, subperiosteal”[MeSH Terms] OR “Subperiosteal implant”[All Fields] OR “subperiosteal implants”[All Fields] OR “juxta-osseous implants”[All Fields].

This electronic search was complemented by:

- Review of the full-text selected articles reference lists.
- Manual searches in the same databases including other free terms such as “custom-made implants”, “Direct Metal Laser Sintering”, “patient-specific implants” or “additively manufactured implants”.
- Grey literature (University of London Online Library, Worldcat, Open Grey, WorldWideScience.org)
- Internet free search.

No restrictions of time were applied. Only articles in English or Spanish were assessed for eligibility. Two authors independently assessed the publications by title and abstract. The inclusion or exclusion criteria for the studies were as follows:

1. *Inclusion criteria:*
2. Clinical studies in humans: Randomized Clinical Trials (RCTs), prospective and retrospective cohort or case-control studies, and case series.

**Table 1** Summary of the search strategy followed to select the articles included in the qualitative synthesis

|  |  |  |          |             |                           |                             |
|--|--|--|----------|-------------|---------------------------|-----------------------------|
| Search strategy  |  |  |          |             |                           |                             |
| Databases: Medline, Scopus, Cochrane Library   |  |  |          |             |                           |                             |
| Date: 11/5/2023  |  |  |          |             |                           |                             |
| Language: English, Spanish   |  |  |          |             |                           |                             |
| Time limits: No  |  |  |          |             |                           |                             |
| Search terms: subperiosteal implants, juxta-osseous implants   |  |  |          |             |                           |                             |
| PICO strategy:   |  |  |          |             |                           |                             |
| In patients with severe bone atrophy (P), do additively manufactured subperiosteal implants (I), compared to subperiosteal implants manufactured following traditional approaches (C), present satisfactory implant survival and complication rates (O)? |  |  |          |             |                           |                             |
|  | Database searched  | Search strategy  | #Records | #Duplicates | #Excluded after screening | #Records included           |
| Identification   | Pubmed-Medline   | Search 1: "dental implantation, subperiosteal"[MeSH Terms] OR "Subperiosteal implant"[All Fields] OR "subperiosteal implants"[All Fields] OR "juxta-osseous implants"[All Fields]  | 389      | –           | 308                       | 11                          |
|  | SCOPUS   | Search 1: "subperiosteal implants" OR "subperiosteal implant" OR "juxta-osseous implants"  | 383      | 1           | 382                       | 0                           |
|  | Cochrane Library   | Search 1: "subperiosteal implants"<br>Search 2: "subperiosteal implant"<br>Search 3: "juxta-osseous implants"  | 20       | 0           | 20                        | 0                           |
|  | Other sources  |  |          |             |                           |                             |
|  | Manual search (including Free terms) in the same databases                                       |  |          |             |                           | 8                           |
|  | Citation searching (references of included studies)  |  |          |             |                           | 2                           |
|  | Internet   |  |          |             |                           | 6                           |
|  | Grey literature (University of London Online Library, Worldcat, Open Grey, WorldWideScience.org) |  |          |             |                           | 4                           |
|  | Total  |  |          |             |                           | 812                         |
|  | Screening  | Records excluded and reasons   |          |             |                           | Total records excluded: 795 |
| - Duplicates<br>- Not focused on the review topic<br>- No clinical studies<br>- Study design: not in accordance with inclusion criteria  |  |  |          |             |                           |                             |
| Eligibility  | Full-text articles excluded with reasons   | - Van den Borre C et al. Radiographic Evaluation of Bone Remodeling after Additively Manufactured Subperiosteal Jaw Implantation (AMSJI) in the Maxilla: A One-Year Follow-Up Study. J Clin Med. 2021 Aug 12;10(16):3542. <sup>a,c</sup><br>- Elsayy MA, et al. Polyetheretherketone subperiosteal implant retaining a maxillary fixed prosthesis: A case series. J Prosthet Dent. 2022 Oct 6:S0022-3913(22)00554-6. <sup>b</sup><br>- Mommaerts MY. Evolutionary steps in the design and biofunctionalization of the additively manufactured sub-periosteal jaw implant 'AMSJI' for the maxilla. Int J Oral Maxillofac Surg. 2019 Jan;48(1):108–114. <sup>a</sup><br>- Jehn P, Spalthoff S, Korn P, Stoetzer M, Gercken M, Gellrich NC, Rahlf B. Oral health-related quality of life in tumour patients treated with patient-specific dental implants. Int J Oral Maxillofac Surg. 2020 Aug;49(8):1067–1072. <sup>a</sup> |          |             | Total records excluded:4  |                             |
|  |  | Reasons<br><sup>a</sup> No information available to answer the PICO question<br><sup>b</sup> Exclusion criteria: Only Implants additively manufactured<br><sup>c</sup> Same patient series as in another already included study  |          |             |                           |                             |
| Included   | Studies included in qualitative synthesis  |  |          |             |                           | 13                          |

3. Subperiosteal implants CAD designed and additively manufactured.
4. *Exclusion criteria*:
5. Case reports.
6. Studies without information related to the measured outcomes.

### Study selection

The study selection was performed by the same two independent reviewers and an additional reviewer acted in case of disagreement. After article selection based on the abstract and the article selection criteria, both reviewers read the complete articles and determined whether they met the inclusion criteria for this review. Agreement in the selection process was calculated using Cohen's kappa coefficient, with a  $\kappa$  value of 0.81 (92.31% of agreement).

### Data collection process

Data from all articles were collected in duplicate by both researchers independently and then pooled in the same worksheet. The following information was extracted from each selected study: year of publication, type of study, number of patients and implants, sex and age of patients, cause of bone defect, inclusion criteria, implant material, manufacturing technology, implant location, design and surface, type of bone fixation, type of prosthetic rehabilitation and retention system, usage of interim prosthesis, design and materials of definitive prosthesis, surgery time, implant fitting rating, follow-up, implant survival, and complications.

### Data synthesis and outcomes

Data from the identified and relevant publications were extracted and, if indicated, presented in evidence tables. The main outcomes analyzed were:

- *Implant survival*. Defined as the presence of the implant in function in the mouth after the end of the follow-up period established in each study.
- *Complications*. Including technical complications affecting both the implant or the prosthesis and all type of biological complication affecting the bone or soft tissues.

### Risk of bias in individual studies

The methodological quality of the included studies was assessed using The National Institutes of Health—"NIH quality assessment tools" for case series and for observational Cohort and Cross-Sectional Studies. Although "NIH quality assessment tools" were initially conceived to help reviewers, these tools have been broadly used in

many recent systematic reviews to assess the study quality [32, 33]. The risk of bias was measured independently by two authors, and in cases of disagreement, a third author participated to solve it.

### Summary measures

All the variables were collected in a database and analyzed with IBM SPSS statistics v. 20.0 (IBM Corp., Armonk—NY, USA). For the univariate description, we employed basic descriptive statistics.

## Results

### Study selection

The initial search provided 792 articles. Additional searches allowed to identify 20 more articles. Before Screening 612 articles were removed. Additionally, 183 articles were also removed after the abstract review. Twelve articles were assessed for eligibility, but after a deep analysis of the article, 4 were excluded for the following reasons:

- No information available to answer the PICO question ( $n=1$ ) [30, 34].
- Not complying with inclusion criteria: Implants additively manufactured ( $n=1$ ) [35].
- Same patient series as in another already included study [36] and no information available to answer the PICO question ( $n=1$ ) [37].

Figure 1 summarizes the study selection process in a *Flow Diagram* adapted from Page et al. [38].

### Study characteristics


The 13 articles finally included in the review [29, 36, 39–49] corresponded to 5 cohort studies (1/5 prospective, 4/5 multicentric) and 8 case series, (1/8 multicentric), that involved a total of 227 patients and the same number of unilateral/bilateral, maxillary/mandibular implants. No RCTs or previous systematic reviews were found during literature search. All the included articles had been published from 2017 onwards.

### Risk of bias within studies

Two articles were multicentric and performed by the same International Group of authors [36, 39] at nearby dates. Possible patient overlapping among both articles is unknown.

### Synthesis of results

The finally selected studies included data from 227 SI placed in 227 patients (121 female / 106 male) with a weighted mean age of 62.4 years. The location of the SI

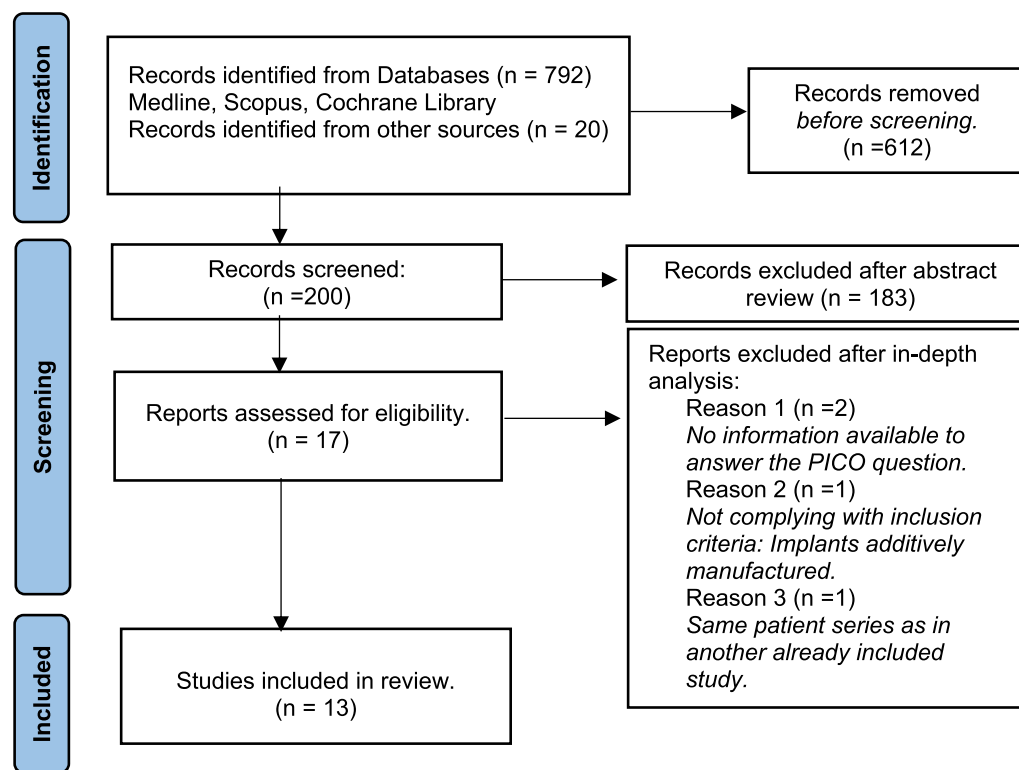

**Fig. 1** Search strategy flow. Adapted from The PRISMA 2020 statement (Page et al. [38])

was specified only for 162 implants (142 maxilla / 20 mandible) and not clearly stated for 65 SI.

The main reason for implantation was bone atrophy. A Cawood–Howell atrophy type V or higher was an inclusion criteria in 5/13 studies, including 94/227 (41.5%) SI. In 24 patients (10.6%) it was clarified that a resective/maxillectomy had been previously performed. One hundred and fourteen patients (50.2%) required a full-arch rehabilitation, 29 (12.8%) a partial restoration and in 84 patients (37%) the type of rehabilitation was not specified (Table 2).

Different implant designs were used across different studies, but in all cases a variable number of osteosynthesis screws were employed to anchor the framework to the bone. All the SI were manufactured in Ti alloys. In the study of Mounir et al. [45], 5 implants included in the group 2 were manufactured in polyether-ether-ketone (PEEK). Data from this 5 PEEK implants were excluded.

The surface in contact with the bone was porous (rough) in 5 studies (83 implants), polished (electroerosion) in 1 study (4 Implants) and not clearly stated in 7 studies (140 implants) (Table 3).

Regarding prosthetic rehabilitation, 113 SI supported a fixed denture, while in 114 patients it was not specified the actual number of fixed and removable dentures.

In 7/13 studies, 144 implants were loaded with interim prostheses at different times after surgery. Prosthetic connection was screw-retained for 104 SI (45.8%) and cemented for 90 SI. For screw-retained restoration, the most common number of connecting posts was 6 (63/104). Definitive prostheses were highly variable in terms of manufacturing techniques, materials, and time of loading (Table 4).

#### Complication rate of SI

After a weighted mean follow-up time of 21.4 months (mean range 1 to 74 months), 97.8% of implants were in function (5 failures reported). In 3 studies [29, 36] (including 22 patients), no complications were reported. Post-operative complications (pain, discomfort, bleeding, swelling) was reported in 17 patients (7.5%), 58 implants (25.6%) presented partial exposure, 12 patients (5.3%) suffered soft tissue infection or persistent infection. The use of a provisional prosthesis was reported in 155 patients. Fracture of the interim prosthesis was reported in 8/155 patients (5.2%). Implant fitting during surgery was assessed in 4 studies [40–42, 44] including 55 SI and rated as satisfactory in 48/55 (87.7%) of the assessed implants (Table 5).



**Table 2** Summary of included studies; study type, demographic data from included patients and inclusion criteria

| Authors                   | Year | Type of study                          | n (patients) | Mean age. (years)                              | Sex      | n (implants) | Cause of bone defect                                 | Inclusion criteria   |
|---------------------------|------|--|--------------|--|----------|--------------|--|--|
| Mangano et al. [40]       | 2020 | Case series                            | 10           | 69.6<br>range:<br>68 to 75                     | 6F/4 M   | 10           | Bone atrophy   | Healthy patients<br>Age > 65 years<br>Nonsmoker<br>Partially edentulous (≥ 2 teeth)<br>Residual bone < 10 mm<br>Acceptable oral hygiene<br>Regenerative bone surgery<br>unwillingness  |
| Van den Borre et al. [36] | 2022 | Prospective Multicenter Study          | 15           | Male: 57.4; SD ± 8.7<br>Female: 62.2; SD ± 3.4 | 7F/8 M   | 15           | Bone atrophy   | Cawood–Howell atrophy ≥ 5<br>Consecutive patients<br>Bilateral placement in the maxilla  |
| Van den Borre et al. [39] | 2023 | Retrospective Multicenter Study        | 40           | Male: 64.6; SD ± 6.7<br>Female: 65.2; SD ± 6.8 | 25F/15 M | 40           | Maxillary defect reconstructions were excluded       | Placement at least one year before assessment<br>122 patients eligible; definitive inclusion by patient and surgeon decisions<br>Maxillary severe atrophy (Cawood–Howell atrophy ≥ 5)  |
| Chamorro Pons et al. [41] | 2021 | Case series                            | 8            | 72.2   | 6F/2 M   | 8            | Bone atrophy   | Cawood–Howell atrophy ≥ 5<br>No systemic contraindications   |
| Cebrián et al. [29]       | 2022 | Case series                            | 4            | 66.2   | 3F/1 M   | 4            | Segmental maxillary oncological defect (due to OSCC) | Patients with segmental maxillary oncological defect that had been reconstructed with a subperiosteal implant  |
| Nemtoi et al. [42]        | 2022 | Retrospective Cohort Multicenter Study | 16           | 61.5<br>Range: 55 to 69                        | 7F/9 M   | 16           | Bone atrophy   | Patient over the age of 55 years<br>Treated with DMLS manufactured subperiosteal implant<br>Equilibrated general and oral health<br>Improved oral hygiene<br>Nonsmoker<br>Available bone height ≤ 10 mm<br>Regenerative bone surgery unwillingness |
| Cerea et al. [43]         | 2018 | Retrospective Multicenter Study        | 70           | 62.8<br>Range: 62 to 79                        | 31F/39 M | 70           | Bone atrophy   | Patient over the age of 60 years<br>Treated with DMLS manufactured subperiosteal implant<br>2-year minimum follow-up<br>Nonsmoker and not bruxist  |

**Table 2** (continued)

| Authors                 | Year | Type of study                | n (patients)           | Mean age. (years)       | Sex     | n (implants)     | Cause of bone defect  | Inclusion criteria  |
|-------------------------|------|------------------------------|------------------------|-------------------------|---------|------------------|---|---|
| Dimitroulis et al. [44] | 2023 | Case series                  | Multicenter Study 21   | 59.1<br>Range: 31 to 80 | 14F/7 M | 21               | Bone atrophy. Maxillectomy (1/21)   | Cawood–Howell atrophy ≥ 5<br>Partial or fully edentulous arches<br>Non smoker<br>Not suffering from a terminal ill or severe medical conditions (as radiotherapy of the jaws)<br>Anterior maxillary bone defect<br>Not enough bone volume to room standard root-form implants (with at least 3 mm of diameter and 8 mm height)<br>No systemic disease or oral pathosis that may affect bone healing<br>No previous grafting procedure at the implant site |
| Mounir et al. [45]      | 2018 | Observational Clinical study | 5*                     | 27.4<br>Range: 18 to 55 | 1F/4 M  | 5                | Bone atrophy  | History of severe bone loss<br>Patients requesting implant-supported dental prosthesis in the absence or impossibility of bone reconstruction by conventional techniques<br>No history of bisphosphonate therapy, psychiatric disorder, alcohol-related diseases, or active smoking   |
| Gellrich et al. [46]    | 2017 | Case series                  | 3                      | 68<br>Range: 55 to 90   | 2F/1 M  | 4                | Bone atrophy (2/3 due to OSCC)  | Cawood–Howell atrophy ≥ 5<br>No head-neck cancer history or previous irradiation<br>No cleft lip or palate, or trauma history   |
| Korn et al. [47]        | 2022 | Case series                  | 10                     | 66<br>Range: 50 to 90   | 7F/3 M  | 13 (3 bilateral) | Bone atrophy  | CLP-associated deformity<br>Maxillary partial or total edentulism   |
| Rahlf et al. [48]       | 2022 | Case series                  | 6                      | 51<br>Range: 18 to 68   | 3F/3 M  | 6                | Cleft lip and palate deformity (CLP)  | Previous tumor resection<br>No history of failed augmentation procedure, trauma, or cleft palate  |
| Korn et al. [49]        | 2021 | Case series                  | Single-center Study 19 | 65<br>Range: 30 to 85   | 9F/10 M | 20 (1 bilateral) | Bone atrophy. 15/20 due to oral malignancy treatment 5/20 due to aggressive oral lesion treatment |   |

\*This study included two groups of implants. Group 1 (5/10 Ti implants) was included. Group 2 1 (5/10 PEEK implants) was excluded



**Table 3** Summary of subperiosteal implants location, characteristics, design, and manufacture

| Authors                   | Implant material | Manufacturing technique  | Implant location (maxilla/mandible)                    | Implant design  | Implant surface (bone face) | Implant fixation   |
|---------------------------|------------------|--|--|---|-----------------------------|--|
| Mangano et al. [40]       | Ti grade V       | DMLS (direct metal laser sintering)  | Posterior mandible                                     | Buccal and lingual arms for implant fixation. Tapered posts for prosthetic cementation  | Porous                      | Osteosynthesis screws Buccal and lingual                                 |
| Van den Borre et al. [36] | Ti grade 23      | Additive manufacture (technique not specified in the text)                           | Maxilla  | 2-piece implants (bilateral) splinted by the prostheses. On each piece: Fixation vestibular arms (2), prosthetic connecting posts (3)                             | Porous                      | Osteosynthesis screws Buccal arms  |
| Van den Borre et al. [39] | Ti grade 23      | Additive manufacture (technique not specified in the text)                           | Maxilla  | 2-piece implants (bilateral) splinted by the prostheses. On each piece: Fixation vestibular arms (2), prosthetic connecting posts (3)                             | Porous                      | Osteosynthesis screws Buccal arms  |
| Chamorro Pons et al. [41] | Ti               | Additive manufacture (technique not specified in the text). Micro-milled connections | Maxilla  | Bilateral main structure with detachable arms (2 or 3 pieces). 6 prosthetic connecting posts (external hexagonal or conical connection). 0.8 mm maximum thickness | NA                          | 14 to 16 osteosynthesis screws (Ø1.5 mm)                                 |
| Cebrián et al. [29]       | Ti               | Sinterization  | Maxilla  | Titanium mesh/plate and prosthetic connecting posts (4 or 6). External hexagonal connection (universal, 4.1 mm)   | NA                          | Osteosynthesis screws  |
| Nemtoi et al. [42]        | Ti               | DMLS (direct metal laser sintering). Post-mechanization                              | 11/16 Maxilla; 5/16 Mandible                           | 0.7 mm thickness. Arms for fixation with osteosynthesis screws  | Rough                       | Osteosynthesis screws  |
| Cerea et al. [43]         | Ti grade V       | DMLS (direct metal laser sintering)  | Maxilla or mandible (no further information available) | Buccal and lingual arms for implant fixation. Tapered posts for prosthetic cementation  | Polished (electroerosion)   | Osteosynthesis screws  |
| Dimitroulis et al. [44]   | Ti               | Laser sintering  | 18/21 Maxilla; 3/21 Mandible                           | Buccal and lingual arms for implant fixation. At least 8 screws placed buccally and additionally, 2 or more in lingual/palatal position. Tapered posts            | NA                          | Osteosynthesis screws (Ø2 mm in the mandible and Ø1.6 mm in the maxilla) |

Table 3 (continued)

| Authors              | Implant material      | Manufacturing technique       | Implant location (maxilla/mandible) | Implant design   | Implant surface (bone face) | Implant fixation                  |
|----------------------|-----------------------|-------------------------------|-------------------------------------|--|-----------------------------|-----------------------------------|
| Mounir et al. [45]   | Ti grade 23 (group 1) | EBM (electron beam melting)   | Anterior maxilla                    | Buccal plate/mesh, buccal holes for the osteosynthesis screws (Ti implants meshed with 2.3 mm holes) and cylindric posts (3 to 6) for prosthetic connection (cemented)                                   | Rough (acid-etching)        | Osteosynthesis screws (Ø2 mm)     |
| Gellrich et al. [46] | Ti grade 23           | SLM (selective laser melting) | Maxilla (1/4), Mandible (3/4)       | Anchorage framework with holes for multiple osteosynthesis screw. Prosthetic posts for internal conventional implant connection, ball attachment system or external conical (telescopic) crow connection | N.A                         | Osteosynthesis screws             |
| Korn et al. [47]     | Ti grade 23           | SLM                           | Maxilla                             | Anchorage framework with holes for multiple osteosynthesis screw. Four connection posts  | N.A                         | Osteosynthesis screws (Ø1.5–2 mm) |
| Rahif et al. [48]    | Ti grade 4            | SLM                           | Maxilla                             | Anchorage framework with holes for multiple osteosynthesis screw. Two to four connection posts   | N.A                         | Osteosynthesis screws (Ø1.5 mm)   |
| Korn et al. [49]     | Ti grade 23           | SLM                           | Maxilla                             | Anchorage framework with holes for multiple osteosynthesis screw. Two to four connection posts   | N.A                         | Osteosynthesis screws (Ø1.2–2 mm) |

**Table 4** Prosthetic rehabilitation; characteristics of temporary and definitive prosthesis

| Authors                   | Type of rehabilitation (partial / full-arch) | Type of prosthesis (fixed / removable) | Provisional prosthesis (use & features)  | Prosthesis fixation                     | Prosthesis impression technique | Definitive prosthesis  |
|---------------------------|--|--|--|---|---------------------------------|--|
| Mangano et al. [40]       | Partial                                      | Fixed                                  | Yes<br>2 sets<br>Milled in PMMA  | Cemented, Temporary cement              | Digital<br>Intraoral scanner    | Zr framework<br>Delivered after 2 months   |
| Van den Borre et al. [36] | Full-arch                                    | Both                                   | Yes<br>Additively manufactured   | Screw-retained, 6 connecting posts      | N/A                             | Overdenture with connecting bar or hybrid FCD<br>Delivered after 2 months  |
| Van den Borre et al. [39] | Full-arch                                    | Both                                   | N/A  | Screw-retained, 6 connecting posts      | N/A                             | Fixed or removable (no further information available)<br>Delivered after 2 months  |
| Chamorro Pons et al. [41] | Full-arch                                    | Fixed                                  | Yes. Premanufactured acrylic prostheses with holes to bond it to temporary abutments. Screw-retained         | Screw-retained, 6 connecting posts      | N/A                             | 6/8 Metal (Cr-Co) CAD/CAM suprastructure veneered with porcelain<br>2/8 Resin hybrid prostheses<br>Delivered after 1.5 to 2 months |
| Cebrián et al. [29]       | Full-arch                                    | Fixed                                  | Yes. Two weeks after surgery   | Screw-retained, 4 or 6 connecting posts | Analogical (open tray)          | Metal () CAD/CAM suprastructure veneered with porcelain. Delivered after 2 months  |
| Nemtoi et al. [42]        | 14/16 full-arch<br>2/16 partial              | N/A                                    | Yes. Within 12 h. After surgery. Fixed acrylic resin prosthesis  | Screw-retained                          | N/A                             | After 6 months<br>(no further information available)   |
| Cerea et al. [43]         | Full-arch or partial                         | Fixed                                  | Yes. Fixed acrylic resin prosthesis. Within 48 h after surgery   | Cemented                                | Analogical (polyvinylsiloxane)  | CAD/CAM metallic suprastructure veneered in ceramic. Delivered after 3–4 months  |
| Dimitroulis et al. [44]   | 18/21 Full-arch; 3/21 partial (maxillary)    | Fixed                                  | Yes. (15/21) CAD/CAM Ti suprastructure and cemented acrylic overlay. Both manufactured using milling methods | Screw-retained                          | N/A                             | Delivered after 2 to 6 months  |
| Mounir et al. [45]        | Partial                                      | Fixed                                  | Acrylic bridges, delivered after 1 month at least<br>No further information available                        | Cemented                                | N/A                             | Delivered after 1 month at least<br>No further information available   |
| Gelrich et al. [46]       | 2/3 Partial, 1/3 Full-arch                   | Removable                              | No provisional prosthesis  | –                                       | Analogical (polyether)          | Delivered after 3–4 months   |
| Korn et al. [47]          | Full-arch                                    | N/A                                    | N/A  | –                                       | Analogical/digital              | N.A. Only 11/14 implants loaded  |
| Rahlf et al. [48]         | 2/6 Partial, 4/6 Full-arch                   | Removable                              | 1/6 provisional prosthesis   | –                                       | N/A                             | N.A. 5/6 implants loaded   |
| Korn et al. [49]          | N/A  | Both                                   | N/A  | –                                       | N/A                             | N/A  |

**Table 5** Follow-up time and summary of clinical outcomes

| Authors                   | Mean surgery time (min) | Follow-up (months)                     | Implant survival         | Implant fitting  | Complications  |
|---------------------------|-------------------------|--|--------------------------|--|--|
| Mangano et al. [40]       | 44.3 ± SD 19.4          | 12                                     | 100%                     | Mean rating: 7 out of 10 SD ± 1.6, median 7, 95% CI 6–8<br>Satisfactory 8/10<br>Insufficient 2/10*<br>*adapted during surgery and placed | 1/10 patient immediate postoperative complications (pain, discomfort, swelling)<br>2/10 patient late complications (provisional restoration fracture)  |
| Van den Borre et al. [36] | N.A                     | 12                                     | 100%                     | N.A  | No complications reported  |
| Van den Borre et al. [39] | N.A                     | 30.1<br>*917 days;<br>SD ± 306.89 days | 100%                     | N.A  | 12/40 postoperative inflammation (i.e., swelling, marked redness, pain)<br>6/40 apparent soft tissue infection, drainage, exploration and/or mechanical debridement needed<br>3/40 required one connecting post removal due to persistent and uncontrollable infection<br>26/40 Partial exposure of the arms not experienced as a functional or esthetic impediment by patients<br>1/40 Mobility of the implant (> 1 mm) |
| Chamorro Pons et al. [41] | 80                      | mean: 18.4<br>range: 4 to 36           | 100%                     | Satisfactory 8/8   | 1/8 needed prosthetic removal and recontouring (soft tissue inflammation/ulceration)   |
| Cebrián et al. [29]       | N.A                     | mean: 20<br>range: 9 to 38             | 100%                     | N.A  | No complications reported  |
| Nemtoi et al. [42]        | 86                      | 12                                     | 93%                      | 5/16 not fully satisfactory<br>Mean satisfaction rate: 4/5   | 3/16 bleeding<br>6/16 implant exposure<br>1/16 implant failure<br>1/16 fracture of temporary prosthesis  |
| Cerea et al. [43]         | N.A                     | 24                                     | 95.8%                    | N.A  | 3/70 failure due to infection<br>4/70 postoperative pain/discomfort/swelling<br>1/70 recurrent infections<br>4/70 fracture of provisional prosthesis<br>2/70 ceramic chipping in the definitive prosthesis   |
| Dimitroulis et al. [44]   | N.A                     | Mean: 22.1<br>range: 5 to 57           | 95% (85.7% success rate) | Satisfactory 21/21   | 1/21 Failure (explanted because of chronic pain)<br>4/21 Salvaged (replacing exposed frames or adding more bone screws)<br>2/21 (considered failures because exposure of the framework even though the device is still functional)   |

**Table 5** (continued)

| Authors              | Mean surgery time (min) | Follow-up (months)           | Implant survival | Implant fitting  | Complications  |
|----------------------|-------------------------|------------------------------|------------------|------------------|--|
| Mounir et al. [45]   | N.A                     | 12                           | 100%             | N.A              | 1/5 wound dehiscence and exposure of the implant. Fully covered subsequently after removal of uncovered rim of the implant<br>5/5 Ti implants showed 1–2 mm exposure of the platform around the posts. (No interference with prosthetic loading or patient dissatisfaction was reported) |
| Gellrich et al. [46] | N.A                     | Mean: 18<br>range: 14 to 21  | 100%             | Satisfactory 3/3 | No complications reported except for partial discomfort/pain in one patient  |
| Korn et al. [47]     | 135                     | Mean: 8.2<br>range: 1 to 29  | 100%             | N.A              | Infection 1/10 patients<br>Exposure of the framework 2/10 patients<br>Screw-loss 1/10 patients   |
| Rahlf et al. [48]    | 146                     | Mean: 18.2<br>range: 6 to 40 | 100%             | N.A              | 6/6 chronic mucositis<br>3/6 Framework exposure around posts   |
| Korn et al. [49]     | 127                     | Mean: 26<br>Range: 6 to 74   | 100%             | N.A              | 1/20 severe infection<br>1/20 exposed screws needed remotion<br>9/20 Exposure of the framework   |

**Table 6** Quality assessment of included articles: *Cohort studies*: (1) Was the research question or objective in this paper clearly stated? (2) Was the study population clearly specified and defined? (3) Was the participation rate of eligible persons at least 50%? (4) Were all the subjects selected or recruited from the same or similar populations (including the same time period)? Were inclusion and exclusion criteria for being in the study prespecified and applied uniformly to all participants? (5) Was a sample size justification, power description, or variance and effect estimates provided? (6) For the analyses in this paper, were the exposure(s) of interest measured prior to the outcome(s) being measured? (7) Was the timeframe sufficient so that one could reasonably expect to see an association between exposure and outcome if it existed? (8) For exposures that can vary in amount or level, did the study examine different levels of the exposure as related to the outcome (e.g., categories of exposure, or exposure measured as continuous variable)? (9) Were the exposure measures (independent variables) clearly defined, valid, reliable, and implemented consistently across all study participants? (10) Was the exposure(s) assessed more than once over time? (11) Were the outcome measures (dependent variables) clearly defined, valid, reliable, and implemented consistently across all study participants? (12) Were the outcome assessors blinded to the exposure status of participants? (13) Was loss to follow-up after baseline 20% or less? (14) Were key potential confounding variables measured and adjusted statistically for their impact on the relationship between exposure(s) and outcome(s)?

#### NIH quality assessment tool for observational cohort and cross-sectional

| Authors                   | Study type                             | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 | 14 | Rating |
|---------------------------|--|---|---|---|---|---|---|---|---|---|----|----|----|----|----|--------|
| Van den Borre et al. [36] | Prospective multicenter study          | * | * | — | * | — | * | * | o | * | o  | *  | o  | —  | —  | Fair   |
| Van den Borre et al. [39] | Retrospective multicenter study        | * | * | — | * | — | * | * | o | * | o  | *  | o  | o  | —  | Fair   |
| Nemtoi et al. [42]        | Retrospective cohort multicenter study | * | * | * | * | — | o | * | o | * | o  | *  | o  | o  | —  | Fair   |
| Cerea et al. [43]         | Retrospective multicenter study        | * | * | o | * | — | o | * | o | * | o  | *  | o  | o  | —  | Fair   |
| Mounir et al. [45]        | Observational clinical study           | * | * | o | * | — | o | * | o | * | o  | *  | o  | o  | —  | Fair   |

\*Yes

—No

° N.A.: not applicable / N.R.: not disclosed

**Table 7** Quality assessment of included articles: *Case series*: (1) Was the study question or objective clearly stated? (2) Was the study population clearly and fully described, including a case definition? (3) Were the cases consecutive? (4) Were the subjects comparable? (5) Was the intervention clearly described? (6) Were the outcome measures clearly defined, valid, reliable, and implemented consistently across all study participants? (7) Was the length of follow-up adequate? (8) Were the statistical methods well-described? (9) Were the results well-described?

**NIH quality assessment tool for case series studies**

| Author                    | Study type                     | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | Rating |
|---------------------------|--------------------------------|---|---|---|---|---|---|---|---|---|--------|
| Mangano et al. [40]       | Case series                    | * | * | ° | * | * | * | * | * | * | Good   |
| Chamorro Pons et al. [41] | Case series                    | * | * | * | * | * | — | — | — | * | Fair   |
| Cebrián et al. [29]       | Case series                    | * | * | — | * | * | — | — | — | * | Fair   |
| Dimitroulis et al. [44]   | Case series multi-center study | * | * | — | * | * | * | * | — | * | Good   |
| Gellrich et al. [45]      | Case series                    | — | * | — | — | — | * | — | — | * | Poor   |
| Korn et al. [46]          | Case series                    | — | * | — | — | — | * | — | — | * | Poor   |
| Rahlf et al. [47]         | Case series                    | * | * | — | — | — | * | * | — | * | Fair   |
| Korn et al. [48]          | Case series                    | * | * | — | * | — | * | * | — | — | Fair   |

\*Yes

—No

° N.A.: not applicable / N.R.: not disclosed

### Risk of bias across studies

Individual study Quality assessment was performed using the NIH—Study Quality Assessment Tool for case series and for cohort studies. Two articles were rated as “Poor”, 2 as “Good” and as “Fair” (Tables 6, 7). Due to the type of study design in selected studies and the great heterogeneity found in methodological aspects, a quantitative analysis followed by meta-analysis was not possible.

### Strength of evidence (SoE)

In absence of randomized studies, the level of evidence was initially rated as “Low”, attending GRADE (Grading of Recommendations, Assessment, Development and Evaluations) system [50]. After assessment of domains that could rate down (Risk of bias, Imprecision, Inconsistency, Indirectness and Publication bias) or rate up (Large magnitude of effect, Dose–Response gradient, Confounding factors) the SoE evaluation was downrated to “Very Low”.

### Discussion

CAD designed additively manufactured SI presented satisfactory survival (97.8%) in the short-term (weighted mean follow-up time 21.4 months; mean range 1 to 74 months), but there is a paucity of data on their success rates and medium- or long-term clinical behavior. Available data are coming only from observational studies (cohort studies and case series), including 227 unilateral/bilateral implants (in 227 patients). From them, 70/227 (31%) came from the same retrospective study [43] and 55/227 (24%) came from two multi-center studies using

same type of implant and performed by the same international team [36, 39]. Another 35/227 (15.4%) came from 3 single-center studies including patients treated with the same type of implant at the same center [47–49].

The most frequent complications reported are those related to soft tissues. Hereby, partial exposure of the framework seems to be the most frequent complication, although this seems not to conditionate the survival in the short-term. New designs could allow to remove exposed parts or prosthetic posts in an easier and safer way than in former designs [13, 39, 44]. Although this fact has not yet been specifically evidenced in the literature, this improvement could positively influence the success of modern SI.

From those patients where the use of a provisional prosthesis was stated, 5.2% suffered a fracture of the interim prosthesis. Despite no further information is available to analyze the reasons, to ensure a good passive fitting of the prosthesis, to carefully adjust the occlusion and to reinforce the framework of interim prosthesis seems advisable for these patients as it is for those wearing conventional root-shape implants [51, 52].

Although the location of the implant was not specified in 65 patients [43], there was a noticeably higher number of maxillary than mandibular implants (142:20). Furthermore, 93/142 (65.4%) of maxillary implants had been manufactured following the same two specific design concept, and material [36, 39, 46–49]. From those stated to have been placed in the mandible (20), 11 supported partial rehabilitations, so the extrapolation of the results



of this review to full-arch mandible SI must be very prudently performed.

Bone implant fitting during surgery (in the 4 assessed studies) [39–42, 44] was satisfactory in mostly all cases. However, it was only assessed in 55 implants and the way of rating this outcome was based on personal feedback and potentially subjective. In those patients where fitting was unsatisfactory, the time of surgery was increased to make the implant fit properly to the bone contour. Dimitroulis et al. [44] noted that longer time (>3 months) between the CT scan and delivery of the SI (what could cause further bone remodeling) or CT slices greater than 1 mm (which reduced the accuracy and tolerance of the device) could influence misfitting.

The main reason for implantation in the selected studies was bone atrophy. A Cawood–Howell atrophy type V or higher was an inclusion criteria in 5/13 studies [36, 39, 41, 44, 47], including 94/227 (41.5%) SI. In 24 patients (10.6%) it was clarified that a resective/maxillectomy had been previously performed. The studies from Mangano et al. [40] and Nemtoi et al. [42] included patients with a residual bone <10 mm and regenerative bone surgery unwillingness on the part of the patient. In these two last studies the advantages and disadvantages of SI over the use of extra-short implants ( $\leq 6.5$  mm) without the need for ancillary bone regenerative procedures could be arguable in the absence of more specific information about each specific case. Extra-short root-shape implants have evidenced in recent systematic reviews and meta-analysis, similar clinical performance to standard-length ones in terms of marginal bone loss (MBL), technical complications or implant survival [52–57]. The possibility of placing an immediate prosthesis, the peculiarities of the type of bone defect in each specific case or the experience degree of the surgeons may have influenced this decision, although the real reasons are unclear. The same can be argued to the study from Mounir et al. [45] where an inclusion criteria was enough bone volume to room standard root-shape implants with at least 3 mm of diameter and 8 mm of length.

Despite SI have a long history, their use is secondary to the use of endo-osseous root-shape implants, both in terms of experience and evidence. Until two decades ago, they were mainly used to support mandibular full-arch removable prostheses [4, 7–9, 58]. In oldest designs, SI were not directly anchored to the bone with osteosynthesis screws or other systems (to avoid movement), were manufactured by casting, required a two-time surgical procedure (first one to take direct impressions of the bone) and good bone–implant fitting was complex to achieve [4, 6–11]. Studies with these oldest designs and materials showed poor clinical results in the medium- or long-term [6]. Between

the 1980s and the 1990s, success rates at 5-year ranging from 90% [10] to 100% [9] were reported but survival rates decreased at 6 years (75%) [10], 10 years (87%) [59] or 13 years (78%) [59]. Furthermore, most of articles did not include other results (in addition to implant survival) that would allow a reliable assessment of the success rate or the degree of patient satisfaction. Considering studies from 90s onwards, a 10-year survival rate of 79% was reported by Yanase et al. [7] and 76% by Bodine et al. [8]. A 6-year evaluation performed by Ferrer et al. [60] revealed a 92.5% success of SI including design innovations and an 84% success for SI with classical designs.

Aforementioned paucity of data does not allow to compare medium- or long-term clinical behavior of modern additively manufactured SI and former ones. In any case, several improvements have been incorporated that could be helpful to improve survival, success and/or patient patient's satisfaction degree, but this is yet to be evidenced. Among these improvements, a better understanding of the biomechanics through finite elements studies has allowed to reduce stress accumulation on bones, implants, abutments, and prosthetic frameworks [61, 62]. Golec [63] anticipated in 1986 the use of CAD/CAM to eliminate the need for surgical bone impression. Since then, several improvements in CBCT definition and additive manufacture refinement were needed to obtain more precise frameworks (reducing misfitting and/or micromovements) [34, 64, 65]. Surface features are also involved in the optimization of SI–bone surface interactions. A higher number of the implants included in this revision were porous (rough) on the bony face to promote osteointegration, and smooth (polish) on the soft tissue face to prevent biofilm colonization [13, 34, 66]. Modern manufacturing and new materials resistance allowed to reduce the thickness of the framework up to 0.7- or 0.8-mm [41, 42]. Further than weight lightening, this reduction seems helpful to prevent exposition. On the other hand, small connections also may lead to more fractures, although the limits of thinning are yet to be studied in more depth.

In relation to SI design too, 4–6 prosthetic posts (implant-prosthesis connectors) were preferred in most studies. All these improvements could have contributed to maintain bone and soft tissue stability. In this sense, Van den Borre et al. [37] performed a radiographic evaluation of modern SI and observed acceptable bone remodeling in the underlying bone (mean negative bone remodeling over six reference points on the crest:  $0.26 \text{ mm} \pm \text{SD } 0.65 \text{ mm}$ ; mean bone remodeling at the supporting bone at the wings and basal frame:  $0.088 \text{ mm} \pm \text{SD } 0.29 \text{ mm}$ ).

No differences in clinical performance between cemented and screw-retained fixed prostheses could be demonstrated. This is not to say that the choice of one retention system or the other lacked clinical significance. From a technical point of view, screw-retained prostheses offer a critical advantage in terms of retrievability. In patients at risk or with a history of previous malignance, screw-retained prosthesis facilitates the mandatory periodical check-up of the tissues underneath fixed rehabilitations [67, 68]. The same rationale can be applied to patients with soft tissue complications, in which screw-retention allows prosthetic removal and recontouring. [42]

Limited information on the performance of SI additively manufactured with other materials different from Ti alloys (PEEK or other materials) is available on the literature. As these materials could be considered very experimental, the group of 5 PEEK SI of the study of Mounir et al. [45] was excluded in the present review. Apart from the data of this study, a case series of 4 edentulous patients was published by Elsayy et al. [35] reporting survival of all the maxillary SI and no complications after a 12-month follow-up period. All the PEEK SI in their study had been manufactured with a 5-axis milling machine, therefore the study did not match the eligibility criteria of the present systematic review.

In summary, modern additively manufactured SI present good survival in the short-time but they still present a notable number of soft tissue complications. Comparing to traditional casted SI, soft-tissue complications could be probably more easily solvable (or containable in extension) as new CAD designs enables a simpler implant trimming and partial removing of the implant. This could reduce the influence of soft-tissue complications on implant survival. Nevertheless, the medium- or long-time clinical behavior is still to be clarified. They present several advantages over traditional casted ones. Better biocompatibility, one-time surgery possibility, a reduction in total mass of the material used, optimization of arms and fixation screws dimensions and number (thus reducing costs and avoiding micromovements) or time of surgery reduction (ensuring a better fitting and avoiding time to re-adapt bone), can be cited among the improvements [13–15]. New finite element method analysis on additively manufactured SI are desirable, to further enhance this advantages and also could be helpful to prevent overextending the implant.

In cases of extreme resorption, SI may be a feasible treatment option in the hands of experienced clinicians. However, in cases where residual bone available allows to room short root-shape implants or standard ones (even with the need for ancillary surgical procedures) the use of SI could be arguable as root-shape implants performance

is further evidenced in the literature. Zygomatic implants are another alternative when the maxillary bone is completely or partially absent if the anatomy of the defect, the remnant bone and the maxillary sinus is favorable. However, zygomatic implants are also considered a complex treatment with significant surgical risk and potential for complications and the success of the treatment is highly dependent on the clinician experience. [69]

In sight of the results of the present study, the use of SI should be based on case selection such as severe atrophy and the impossibility (or unwillingness on the part of the patient) to conduct microvascular bone reconstruction or even patients that have a reduced expected lifespan.

A significant limitation of the present review is the absence of RCTs, prospective studies or other studies with a higher level of evidence in the available literature. A meta-analysis was not possible to obtain, due to this and the great heterogeneity between studies. On the other hand, no previous systematic review has been conducted on the topic to the best knowledge of the authors, and the results obtained could encourage to perform new well-designed studies to clarify the important lack of information in some key points for clinical practice. In sight of the results of the present systematic review, some treatment recommendations for former SI in older studies could be partially outdated.

## Conclusions

Subperiosteal implants have been used for decades, but lost relevance among clinicians due former poor clinical performance. Improvements through new technologies development have brought them to a new scenario. Based on the available studies (observational), “modern” CAD designed, and additively manufactured SI presented a satisfactory survival in the short time. However, further studies are needed to ascertain the success rate and the clinical behavior in the medium- and long-term. It would also be desirable to conduct further studies on CAD designed SI manufactured with the most modern subtractive manufacturing methods in view of the limited available clinical information.

Partial exposure was the most common complication reported. Post-operative complications, soft-tissue infection and interim prosthesis fracture were other remarkable complications reported. New SI designs may be helpful to prevent complications, but there is a need to strengthen the evidence with new clinical studies.

## Acknowledgements

Not applicable.

### Author contributions

All authors have made substantial contributions to the conception or design of the work or the acquisition, analysis, or interpretation of data for the work; and drafting the work or revising it critically for important intellectual content; and have given final approval of the version to be published; and agree to be accountable for all aspects of the work in ensuring that questions related to the accuracy or integrity of any part of the work are appropriately investigated and resolved.

### Funding

This work was supported by Horizon 2020 Framework Program [Grant number 953134].

### Availability of data and materials

The datasets used and/or analyzed during the current study are available from the corresponding author on reasonable request.

### Declarations

#### Ethics approval and consent to participate

Not applicable.

#### Consent for publication

Not applicable.

#### Competing interests

EA is the Scientific Director of BTI Biotechnology Institute, a dental implant company that investigates in the fields of oral implantology and PRGF-Endoret technology. MHA is a researcher at BTI Biotechnology Institute. AE is a researcher at the Eduardo Anitua Foundation. CS has no conflicts of interest.

#### Author details

<sup>1</sup>University Institute for Regenerative Medicine and Oral Implantology, UIRMI (UPV/EHU-Fundación Eduardo Anitua), Jose Maria Cagigal Kalea, 19, 01007 Vitoria-Gasteiz, Araba, Spain. <sup>2</sup>University of the Basque Country UPV/EHU and University Institute for Regenerative Medicine and Oral Implantology, UIRMI (UPV/EHU-Fundación Eduardo Anitua), Vitoria, Spain. <sup>3</sup>Department of Cranio-Maxillofacial Surgery, Kepler Universitätsklinikum, Linz, Austria. <sup>4</sup>BTI-Biotechnology Institute, Vitoria, Spain.

Received: 12 June 2023 Accepted: 11 January 2024

Published online: 05 February 2024

### References

- Dahl G. Om möjligheten för implantation i ka'ken av metallskelett som bas eller retention för fasta eller avtagbarproteser. *Odontol Tidskr.* 1943;51:440–9.
- Goldberg NI, Gershkoff A. The implant lower denture. *Dent Dig.* 1949;55:490–5.
- Buser D, Sennerby L, De Bruyn H. Modern implant dentistry based on osseointegration: 50 years of progress, current trends and open questions. *Periodontol.* 2000;2017(73):7–21.
- Moore DJ, Hansen PA. A descriptive 18-year retrospective review of subperiosteal implants for patients with severely atrophied edentulous mandibles. *J Prosthet Dent.* 2004;92(2):145–50.
- Gore D, Frazer RQ, Kovarik RE, Yepes JE. Vitallium. *J Long Term Eff Med Implants.* 2005;15(6):673–86.
- Schou S, Pallesen L, Hjørting-Hansen E, Pedersen CS, Fibaek B. A 41-year history of a mandibular subperiosteal implant. *Clin Oral Implants Res.* 2000;11(2):171–8.
- Yanase RT, Bodine RL, Tom JF, White SN. The mandibular subperiosteal implant denture: a prospective survival study. *J Prosthet Dent.* 1994;71(4):369–74.
- Bodine RL, Yanase RT, Bodine A. Forty years of experience with subperiosteal implant dentures in 41 edentulous patients. *J Prosthet Dent.* 1996;75(1):33–44.
- Golec TS. The mandibular full subperiosteal implant—clinical review of 100 cases. *Dent Surv.* 1980;56(4):32–8.
- Young L Jr, Michel JD, Moore DJ. A twenty-year evaluation of subperiosteal implants. *J Prosthet Dent.* 1983;49(5):690–4.
- Linkow LI, Ghalili R. Critical design errors in maxillary subperiosteal implants. *J Oral Implantol.* 1998;24(4):198–205.
- Nguyen TM, Caruhal JB, Khonsari RH. A subperiosteal maxillary implant causing severe osteolysis. *J Stomatol Oral Maxillofac Surg.* 2018;119(6):523–5.
- Mommaerts MY. Additively manufactured sub-periosteal jaw implants. *Int J Oral Maxillofac Surg.* 2017;46(7):938–40.
- Carnicero A, Peláez A, Restoy-Lozano A, Jacquot I, Perera R. Improvement of an additively manufactured subperiosteal implant structure design by finite elements based topological optimization. *Sci Rep.* 2021;11(1):15390.
- Castrillo G, Carnicero A, Perera R. Submodelling approach to screw-to-bone interaction in additively manufactured subperiosteal implant structures. *Int J Numer Method Biomed Eng.* 2023;39(2): e3672.
- Bai L, Zheng L, Ji P, Wan H, Zhou N, Liu R, Wang C. Additively manufactured lattice-like subperiosteal implants for rehabilitation of the severely atrophic ridge. *ACS Biomater Sci Eng.* 2022;8(2):912–20.
- Gellrich NC, Rahlf B, Zimmerer R, Pott PC, Rana M. A new concept for implant-borne dental rehabilitation; how to overcome the biological weak-spot of conventional dental implants? *Head Face Med.* 2017;13(1):17.
- Spalthoff S, Borrmann M, Jehn P, Rahlf B, Gellrich NC, Korn P. Comparison of conventional and digital workflow for dental rehabilitation with a novel patient-specific framework implant system: an experimental dataset evaluation. *Int J Implant Dent.* 2022;8(1):4.
- Yan Q, Wu X, Su M, Hua F, Shi B. Short implants ( $\leq 6$  mm) versus longer implants with sinus floor elevation in atrophic posterior maxilla: a systematic review and meta-analysis. *BMJ Open.* 2019;9(10): e029826.
- Anitua E, Alkhraisat MH. 15-year follow-up of short dental implants placed in the partially edentulous patient: mandible vs maxilla. *Ann Anat.* 2019;222:88–93.
- Cruz RS, Lemos CAA, de Batista VES, Yogui FC, Oliveira HFF, Verri FR. Narrow-diameter implants versus regular-diameter implants for rehabilitation of the anterior region: a systematic review and meta-analysis. *Int J Oral Maxillofac Surg.* 2020. <https://doi.org/10.1016/j.ijom.2020.10.001>.
- Raghoobar GM, Onclin P, Boven GC, Vissink A, Meijer HJA. Long-term effectiveness of maxillary sinus floor augmentation: a systematic review and meta-analysis. *J Clin Periodontol.* 2019;46(Suppl 21):307–18.
- Antonoglou GN, Stavropoulos A, Samara MD, Ioannidis A, Benic GI, Papageorgiou SN, Sándor GK. Clinical performance of dental implants following sinus floor augmentation: a systematic review and meta-analysis of clinical trials with at least 3 years of follow-up. *Int J Oral Maxillofac Implants.* 2018;33:e45–65.
- Robert L, Aloy-Prósper A, Arias-Herrera S. Vertical augmentation of the atrophic posterior mandibular ridges with onlay grafts: intraoral blocks vs. guided bone regeneration. *Systematic review. J Clin Exp Dent.* 2023;15(5):e357–65.
- Hameed MH, Gul M, Ghafoor R, Khan FR. Vertical ridge gain with various bone augmentation techniques: a systematic review and meta-analysis. *J Prosthodont.* 2019;28(4):421–7.
- Anitua E, Anitua B, Alkhraisat MH, Piñas L, Torre A, Eguía A. Dental implants survival after nasal floor elevation: a systematic review. *J Oral Implantol.* 2022;48(6):595–603.
- Tavelli C, Tedesco A. Survival and complication rate of zygomatic implants: a systematic review. *J Oral Implantol.* 2022. <https://doi.org/10.1563/aaid-joi-D-22-00008>.
- King S, Butterworth C. Attitudes regarding zygomatic implant surgical and prosthodontic techniques—a cohort questionnaire study. *Oral Maxillofac Surg.* 2022;26(3):439–45.
- Cebrián Carretero JL, Del Castillo Pardo de Vera JL, Montesdeoca García N, Garrido Martínez P, Pampín Martínez MM, Aragón Niño I, Navarro Cuéllar I, Navarro Cuéllar C. Virtual surgical planning and customized subperiosteal titanium maxillary implant (CSTMI) for three dimensional reconstruction and dental implants of maxillary defects after oncological resection: case series. *J Clin Med.* 2022;11(15):4594.
- Jehn P, Spalthoff S, Korn P, Stoetzer M, Gercken M, Gellrich NC, Rahlf B. Oral health-related quality of life in tumour patients treated with patient-specific dental implants. *Int J Oral Maxillofac Surg.* 2020;49(8):1067–72.
- Moher D, Liberati A, Tetzlaff J, Altman DG, The PRISMA Group. Preferred reporting items for systematic reviews and meta-analyses: the PRISMA statement. *PLoS Med.* 2009. <https://doi.org/10.1371/journal.pmed.1000097>.

32. Ebell MH, Siwek J, Weiss BD, Woolf SH, Susman J, Ewigman B, Bowman M. Strength of recommendation taxonomy (SORT): a patient-centered approach to grading evidence in the medical literature. *J Am Board Fam Pract.* 2004;17:59–67.
33. Ma LL, Wang YY, Yang ZH, Huang D, Weng H, Zeng XT. Methodological quality (risk of bias) assessment tools for primary and secondary medical studies: what are they and which is better? *Mil Med Res.* 2020;7:7.
34. Mommaerts MY. Evolutionary steps in the design and biofunctionalization of the additively manufactured sub-periosteal jaw implant 'AMSJI' for the maxilla. *Int J Oral Maxillofac Surg.* 2019;48(1):108–14.
35. Elsayw MA, Elgamel ME, Ahmed WM, El-Daker MA, Hegazy SA. Poly-etheretherketone subperiosteal implant retaining a maxillary fixed prosthesis: a case series. *J Prosthet Dent.* 2022. <https://doi.org/10.1016/j.prosdent.2022.08.027>.
36. Van den Borre C, Rinaldi M, De Neef B, Loomans NAJ, Nout E, Van Doorne L, Naert I, Politis C, Schouten H, Klomp G, Beckers L, Freilich MM, Mommaerts MY. Patient- and clinician-reported outcomes for the additively manufactured sub-periosteal jaw implant (AMSJI) in the maxilla: a prospective multi-centre one-year follow-up study. *Int J Oral Maxillofac Surg.* 2022;51(2):243–50.
37. Van den Borre C, Rinaldi M, De Neef B, Loomans NAJ, Nout E, Van Doorne L, Naert I, Politis C, Schouten H, Klomp G, Beckers L, Freilich MM, Mommaerts MY. Radiographic evaluation of bone remodeling after additively manufactured subperiosteal jaw implantation (AMSJI) in the maxilla: a one-year follow-up study. *J Clin Med.* 2021;10(16):3542.
38. Page MJ, McKenzie JE, Bossuyt PM, Boutron I, Hoffmann TC, Mulrow CD, Shamseer L, Tetzlaff JM, Akl EA, Brennan SE, Chou R, Glanville J, Grimshaw JM, Hróbjartsson A, Lalu MM, Li T, Loder EW, Mayo-Wilson E, McDonald S, McGuinness LA, Stewart LA, Thomas J, Tricco AC, Welch VA, Whiting P, Moher D. The PRISMA 2020 statement: an updated guideline for reporting systematic reviews. *BMJ.* 2021;372: n71.
39. Van den Borre C, De Neef B, Loomans NAJ, Rinaldi M, Nout E, Bouvry P, Naert I, Mommaerts MY. Patient satisfaction and impact on oral health after maxillary rehabilitation using a personalized additively manufactured subperiosteal jaw implant (AMSJI). *J Pers Med.* 2023;13(2):297.
40. Mangano C, Bianchi A, Mangano FG, Dana J, Colombo M, Solop I, Admakin O. Custom-made 3D printed subperiosteal titanium implants for the prosthetic restoration of the atrophic posterior mandible of elderly patients: a case series. *3D Print Med.* 2020;6(1):1.
41. Chamorro-Pons M, Arias-Gallo J, Margarit-Pérez L, Demaría-Martínez G, Ciudad-Vicario A. Implantes subperiosteos personalizados para la rehabilitación completa del maxilar superior atrofico. Revisión de una serie clínica de 8 casos. *Rev Esp Ciruj Oral y Maxilofac.* 2021;43(4):140–8.
42. Nemtoi A, Covrig V, Nemtoi A, Stoica G, Vatau R, Haba D, Zetu I. Custom-made direct metal laser sintering titanium subperiosteal implants in oral and maxillofacial surgery for severe bone-deficient patients-a pilot study. *Diagnostics (Basel).* 2022;12(10):2531.
43. Cerea M, Dolcini GA. Custom-made direct metal laser sintering titanium subperiosteal implants: a retrospective clinical study on 70 patients. *Biomed Res Int.* 2018;2018:5420391.
44. Dimitroulis G, Gupta B, Wilson I, Hart C. The atrophic edentulous alveolus. A preliminary study on a new generation of subperiosteal implants. *Oral Maxillofac Surg.* 2023;27(1):69–78.
45. Mounir M, Atef M, Abou-Elfetouh A, Hakam MM. Titanium and polyether ether ketone (PEEK) patient-specific sub-periosteal implants: two novel approaches for rehabilitation of the severely atrophic anterior maxillary ridge. *Int J Oral Maxillofac Surg.* 2018;47(5):658–64.
46. Gellrich NC, Zimmerer RM, Spalthoff S, Jehn P, Pott PC, Rana M, Rahlf B. A customised digitally engineered solution for fixed dental rehabilitation in severe bone deficiency: a new innovative line extension in implant dentistry. *J Craniomaxillofac Surg.* 2017;45(10):1632–8.
47. Korn P, Gellrich NC, Spalthoff S, Jehn P, Eckstein F, Lentge F, Zeller AN, Rahlf B. Managing the severely atrophic maxilla: farewell to zygomatic implants and extensive augmentations? *J Stomatol Oral Maxillofac Surg.* 2022;123(5):562–5.
48. Rahlf B, Korn P, Zeller AN, Spalthoff S, Jehn P, Lentge F, Gellrich NC. Novel approach for treating challenging implant-borne maxillary dental rehabilitation cases of cleft lip and palate: a retrospective study. *Int J Implant Dent.* 2022;8(1):6.
49. Korn P, Gellrich NC, Jehn P, Spalthoff S, Rahlf B. A new strategy for patient-specific implant-borne dental rehabilitation in patients with extended maxillary defects. *Front Oncol.* 2021;11: 718872.
50. Guyatt GH, Oxman AD, Vist GE, Kunz R, Falck-Ytter Y, Alonso-Coello P, Schünemann HJ, GRADE Working Group. GRADE: an emerging consensus on rating quality of evidence and strength of recommendations. *BMJ.* 2008;336(7650):924–6.
51. De Bruyn H, Raes S, Ostman PO, Cosyn J. Immediate loading in partially and completely edentulous jaws: a review of the literature with clinical guidelines. *Periodontol 2000.* 2014;66(1):153–87.
52. Sadid-Zadeh R, Zirkel C, Makwoka S, Li R. Fracture strength of interim CAD/CAM and conventional partial fixed dental prostheses. *J Prosthodont.* 2021;30(8):720–4.
53. Nisand D, Picard N, Rocchietta I. Short implants compared to implants in vertically augmented bone: a systematic review. *Clin Oral Implants Res.* 2015;26:170–9.
54. Badaró MM, Mendoza Marin DO, Pauletto P, Simek Vega Gonçalves TM, Porporatti AL, De Luca Canto G. Failures in single extra-short implants ( $\leq 6$  mm): a systematic review and meta-analysis. *Int J Oral Maxillofac Implants.* 2021;36:669–89.
55. Torres-Alemay A, Fernández-Estevan L, Agustín-Panadero R, Montiel-Company JM, Labaig-Rueda C, Mañes-Ferrer JF. Clinical behavior of short dental implants: systematic review and meta-analysis. *J Clin Med.* 2020;9:3271.
56. Vetromilla BM, Mazzetti T, Pereira-Cenci T. Short versus standard implants associated with sinus floor elevation: an umbrella review of meta-analyses of multiple outcomes. *J Prosthet Dent.* 2021;126:503–11.
57. Lemos CA, Ferro-Alves ML, Okamoto R, Mendonça MR, Pellizzer EP. Short dental implants versus standard dental implants placed in the posterior jaws: a systematic review and meta-analysis. *J Dent.* 2016;47:8–17.
58. Garefis PN. Complete mandibular subperiosteal implants for edentulous mandibles. *J Prosthet Dent.* 1978;39(6):670–7.
59. James RA, Lozada JL, Truitt PH, Foust BE, Jovanovic SA. Subperiosteal implants. *CDA J.* 1988;16(1):10–4.
60. Ferrer F. A newly designed partial subperiosteal implant and the classical design: a comparative study. *P R Health Sci J.* 1994;13(3):183–90.
61. Keleş HG, Karaca Ç. Comparison of stress distribution among standard dental implants placed in grafted bone, zygomatic implants, and subperiosteal implants in the atrophic edentulous maxilla: 3D finite element analysis. *Int J Oral Maxillofac Implants.* 2023;38(2):347–56.
62. Altuparmak N, Polat S, Onat S. Finite element analysis of the biomechanical effects of titanium and Cfr-peek additively manufactured subperiosteal jaw implant (AMSJI) on maxilla. *J Stomatol Oral Maxillofac Surg.* 2023. <https://doi.org/10.1016/j.jormas.2022.09.011>.
63. Golec TS. CAD-CAM multiplanar diagnostic imaging for subperiosteal implants. *Dent Clin North Am.* 1986;30(1):85–95.
64. Valenti C, Isabella Federici M, Masciotti F, Marinucci L, Xhimitiku I, Cianetti S, Pagano S. Mechanical properties of 3D-printed prosthetic materials compared with milled and conventional processing: a systematic review and meta-analysis of in vitro studies. *J Prosthet Dent.* 2022. <https://doi.org/10.1016/j.prosdent.2022.06.008>.
65. Fokas G, Vaughn VM, Scarfe WC, Bornstein MM. Accuracy of linear measurements on CBCT images related to presurgical implant treatment planning: a systematic review. *Clin Oral Implants Res.* 2018;29(Suppl 16):393–415.
66. Ardhan R, Diana R, Pidhatika B. How *Porphyromonas gingivalis* navigate the map: the effect of surface topography on the adhesion of *Porphyromonas gingivalis* on biomaterials. *Materials (Basel).* 2022;15(14):4988.
67. Anitua E, Alkhraisat MH, Piñas L, Torre A, Eguia A. Implant-prosthetic treatment in patients with oral lichen planus: a systematic review. *Spec Care Dentist.* 2022;42(1):60–72.
68. Anitua E, Alkhraisat MH. Clinical performance of short dental implants supporting single crown restoration in the molar-premolar region: cement versus screw retention. *Int J Oral Maxillofac Implants.* 2019;34:969–76.
69. Al-Nawas B, Aghaloo T, Aparicio C, Bedrossian E, Brecht L, Brennand-Roper M, Chow J, Davó R, Fan S, Jung R, Kämmerer PW, Kumar VV, Lin WS, Malevez C, Morton D, Pijpe J, Polido WD, Raghoobar GM, Stumpel LJ, Tuminelli FJ, Verdino JB, Vissink A, Wu Y, Zarrine S. ITI consensus report on zygomatic implants: indications, evaluation of surgical techniques and long-term treatment outcomes. *Int J Implant Dent.* 2023;9(1):28.

## Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.